

134071-44-6P2870458


7.787
7.767
7.473
7.452
7.444
7.439
7.404
7.384
7.375
7.264
7.237
7.231
7.216
7.210
6.884
6.849
4.454
4.417
4.352
4.315
4.275
4.260
4.246
4.233
4.218
3.804
3.788
3.782
3.775
3.766
3.761
3.748
3.735
3.609
3.598
3.588
3.576
3.455
3.439
3.429
3.413
2.479



Current Data Parameters
NAME 134071-44-6P2870458
EXFNO 1
PROCNO 1

F2 - Acquisition Parameters
Date_ 20231211
Time 15.01 h
INSTRUM Avance neo 400
PROBHD Z163739_0670 (
PULPROG zg30
TD 65536
SOLVENT CDCl3
NS 4
DS 2
SWH 8196.722 Hz
FIDRES 0.250144 Hz
AQ 3.9976359 sec
RG 101
DW 61.000 usec
DE 13.89 usec
TE 299.1 K
D1 1.00000000 sec
TD0 1
SFO1 400.1324708 MHz
NUC1 1H
PO 2.67 usec
P1 8.00 usec
PLW1 22.77899933 W

F2 - Processing parameters
SI 65536
SF 400.1300083 MHz
WDW EM
SSB 0
LB 0.30 Hz
GB 0
PC 1.00

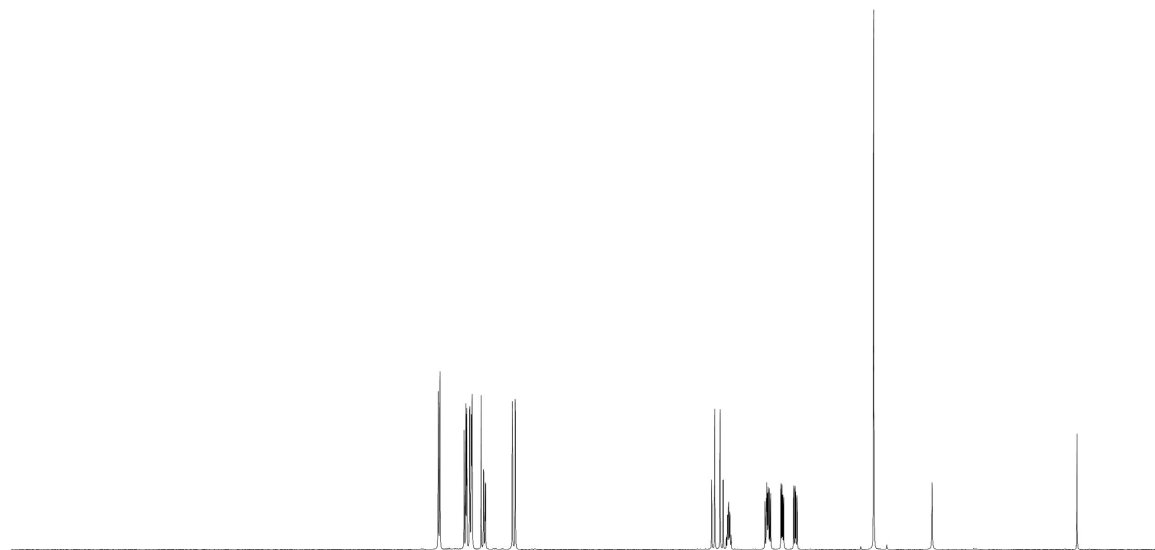

12 11 10 9 8 7 6 5 4 3 2 1 0 ppm

1.950
1.951
2.948
1.021
1.954

1.019
1.006
1.013
2.030
1.023
1.015

3.000