


13534-99-1P2546963



8.026
8.022
8.014
8.010
7.660
7.657
7.641
7.637
7.285
6.558
6.545
6.538
6.526
6.515
— 5.100

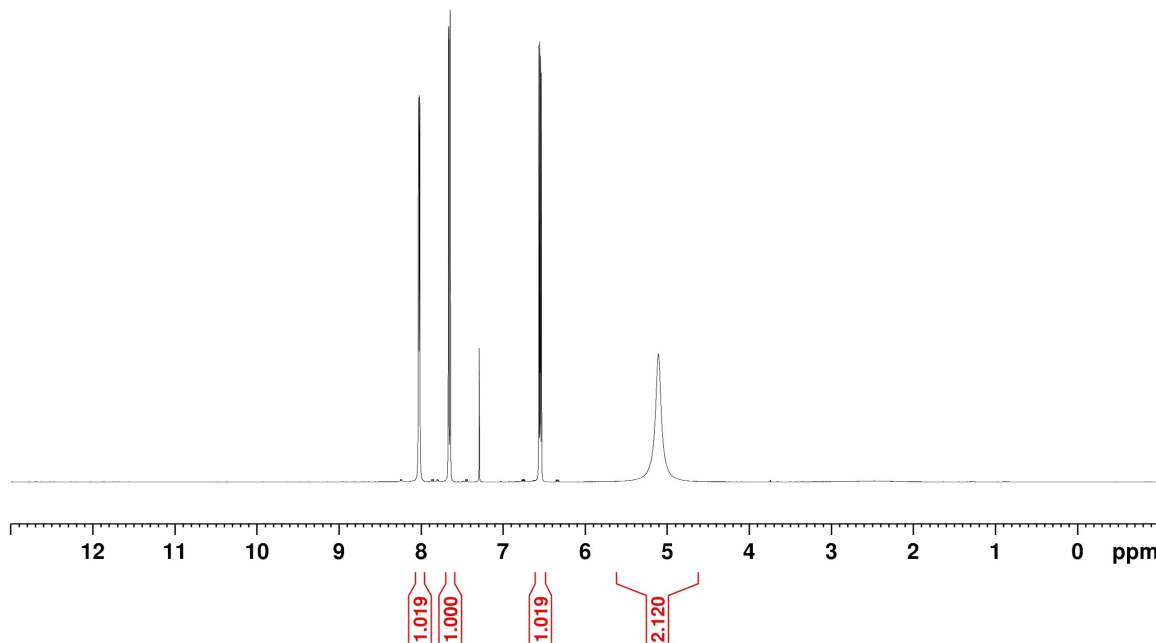

Current Data Parameters
NAME 13534-99-1P2546963
EXFNO 1
PROCNO 1

F2 - Acquisition Parameters
Date_ 20230313
Time 13.50 h
INSTRUM Avance neo 400
PROBHD Z163739_0670 (
PULPROG zg30
TD 65536
SOLVENT CDCl3
NS 4
DS 2
SWH 8196.722 Hz
FIDRES 0.250144 Hz
AQ 3.9976359 sec
RG 101
DW 61.000 usec
DE 13.89 usec
TE 297.7 K
D1 1.00000000 sec
TD0 1
SF01 400.1324708 MHz
NUC1 1H
PO 2.67 usec
P1 8.00 usec
PLW1 22.77899933 W

F2 - Processing parameters
SI 65536
SF 400.1300000 MHz
WDW EM
SSB 0
LB 0.30 Hz
GB 0
PC 1.00