

140-11-4P2518371

7.424
7.401
7.392
7.377
7.371
7.366
7.356
7.343
7.284

5.144

2.135


1.738



Current Data Parameters
NAME 140-11-4P2518371
EXFNO 1
PROCNO 1

F2 - Acquisition Parameters
Date_ 20230321
Time 17.35 h
INSTRUM Avance neo 400
PROBHD Z163739_0670 (
PULPROG zg30
TD 65536
SOLVENT CDCl3
NS 4
DS 2
SWH 8196.722 Hz
FIDRES 0.250144 Hz
AQ 3.9976959 sec
RG 45.2
DW 61.000 usec
DE 13.89 usec
TE 298.0 K
D1 1.00000000 sec
TD0 1
SFO1 400.1324708 MHz
NUC1 1H
PO 2.67 usec
P1 8.00 usec
PLW1 22.77899933 W

F2 - Processing parameters
SI 65536
SF 400.1300000 MHz
WDW EM
SSB 0
LB 0.30 Hz
GB 0
PC 1.00

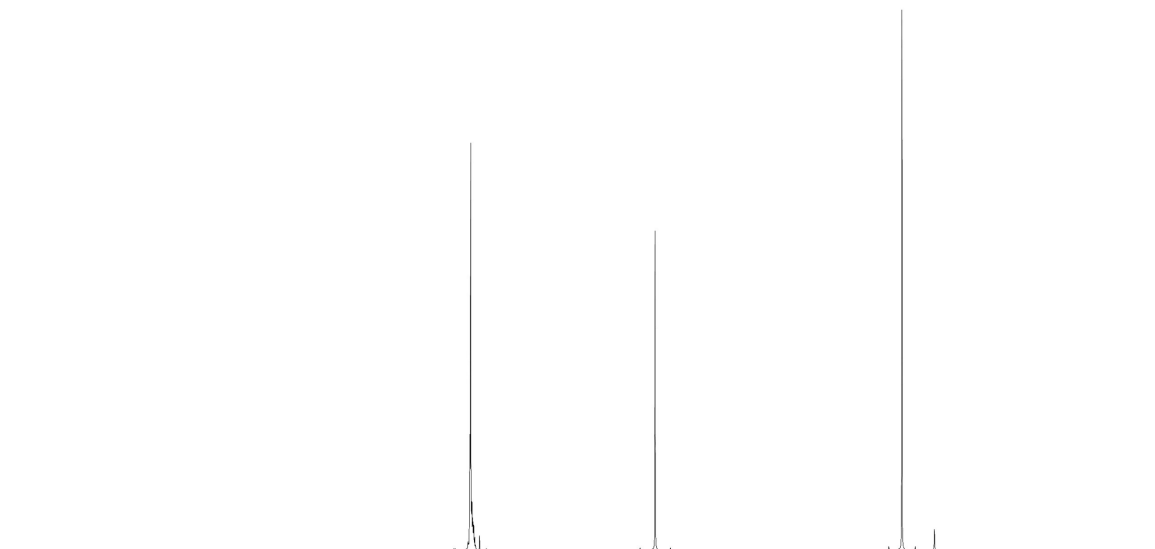

12

11

10

9

8

7

6

5

4

3

2

1

0

ppm

5.000

2.052

3.072