

14246-53-8P2625154

8.101
8.087
8.072


3.719
3.705
2.508
2.504
2.499
2.120
2.102
2.083
1.518
1.500
1.483
1.466
1.311
1.294
1.276
1.244
0.875
0.858



Current Data Parameters
NAME 14246-53-8P2625154
EXFNO 1
PROCNO 1

F2 - Acquisition Parameters
Date_ 20230524
Time 11.55 h
INSTRUM Avance nec 400
PROBHD Z163739_0670 (
PULPROG zg30
TD 65536
SOLVENT DMSO
NS 4
DS 2
SWH 8196.722 Hz
FIDRES 0.250144 Hz
AQ 3.9976359 sec
RG 57
DW 61.000 usec
DE 13.89 usec
TE 297.7 K
D1 1.00000000 sec
TD0 1
SFO1 400.1324708 MHz
NUC1 1H
PO 2.67 usec
P1 8.00 usec
PLW1 22.77899933 W

F2 - Processing parameters
SI 65536
SF 400.1300021 MHz
WDW EM
SSB 0
LB 0.30 Hz
GB 0
PC 1.00

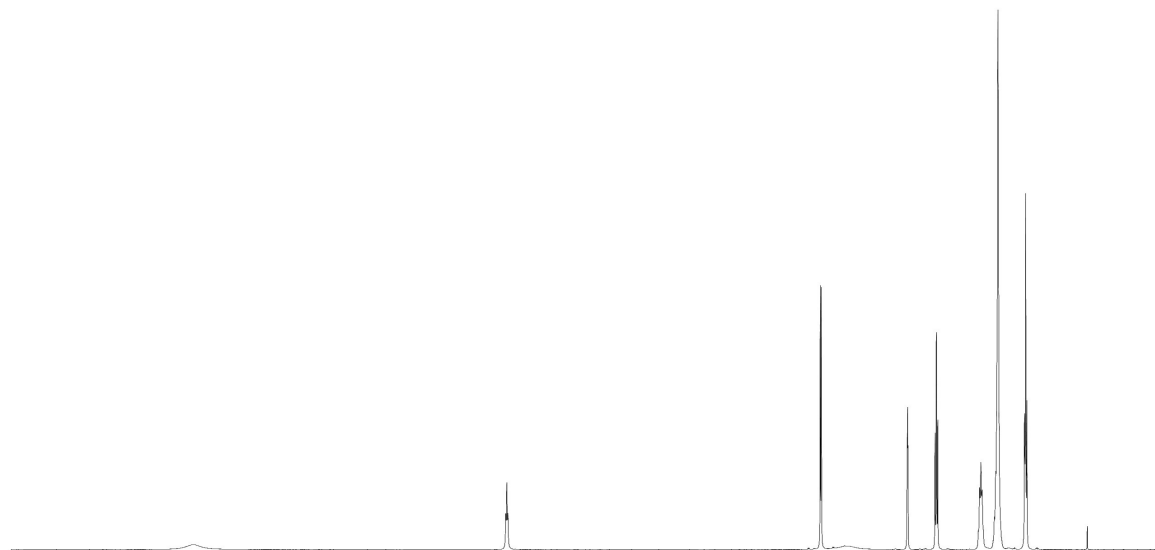

14 13 12 11 10 9 8 7 6 5 4 3 2 1 0 ppm

0.790

1.000

2.049

2.010

2.012

8.086

2.993