

150-60-7P2811433

7.334
7.330
7.326
7.313
7.309
7.294
7.281
7.278
7.274
7.267
7.260
7.251
7.241
7.237
7.231
7.221

— 3.590

— 1.511


— -0.000



Current Data Parameters
NAME 150-60-7P2811433
EXFNO 1
PROCNO 1

F2 - Acquisition Parameters
Date_ 20231024
Time 17.28 h
INSTRUM Avance neo 400
PROBHD Z163739_0670 (
PULPROG zg30
TD 65536
SOLVENT CDCl3
NS 4
DS 2
SWH 8196.722 Hz
FIDRES 0.250144 Hz
AQ 3.9976959 sec
RG 57
DW 61.000 usec
DE 13.89 usec
TE 296.9 K
D1 1.00000000 sec
TD0 1
SFO1 400.1324708 MHz
NUC1 1H
PO 2.67 usec
P1 8.00 usec
PLW1 22.77899933 W

F2 - Processing parameters
SI 65536
SF 400.1300215 MHz
WDW EM
SSB 0
LB 0.30 Hz
GB 0
PC 1.00

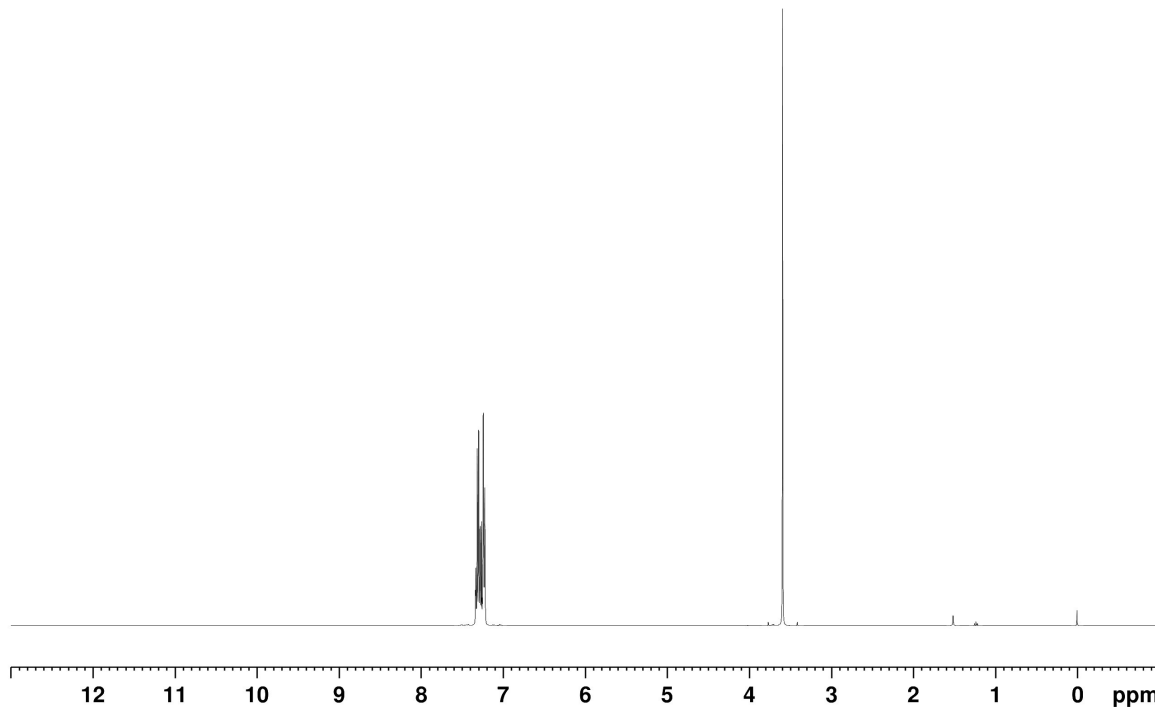

5.000
5.162

4.203