

24589-77-3P2495488

7.866
7.860
7.855
7.843
7.838
7.831
6.915
6.909
6.903
6.891
6.886
6.880


— 4.700



Current Data Parameters
NAME 24589-77-3P2495488
EXFNO 1
PROCNO 1

F2 - Acquisition Parameters
Date_ 20230328
Time 13.02 h
INSTRUM Avance neo 400
PROBHD Z163739_0670 (
PULPROG zg30
TD 65536
SOLVENT D2O
NS 4
DS 2
SWH 8196.722 Hz
FIDRES 0.250144 Hz
AQ 3.9976359 sec
RG 101
DW 61.000 usec
DE 13.89 usec
TE 297.1 K
D1 1.00000000 sec
TD0 1
SFO1 400.1324708 MHz
NUC1 1H
PO 2.67 usec
P1 8.00 usec
PLW1 22.77899933 W

F2 - Processing parameters
SI 65536
SF 400.1300000 MHz
WDW EM
SSB 0
LB 0.30 Hz
GB 0
PC 1.00

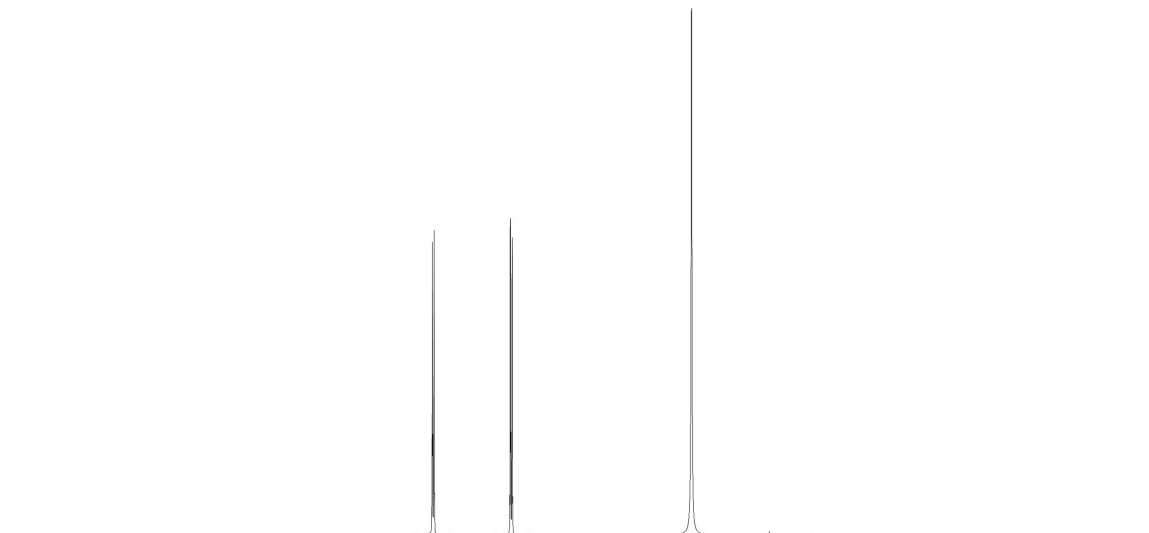

12 11 10 9 8 7 6 5 4 3 2 1 0 ppm

2.000

2.001