


2687-94-7P2525078

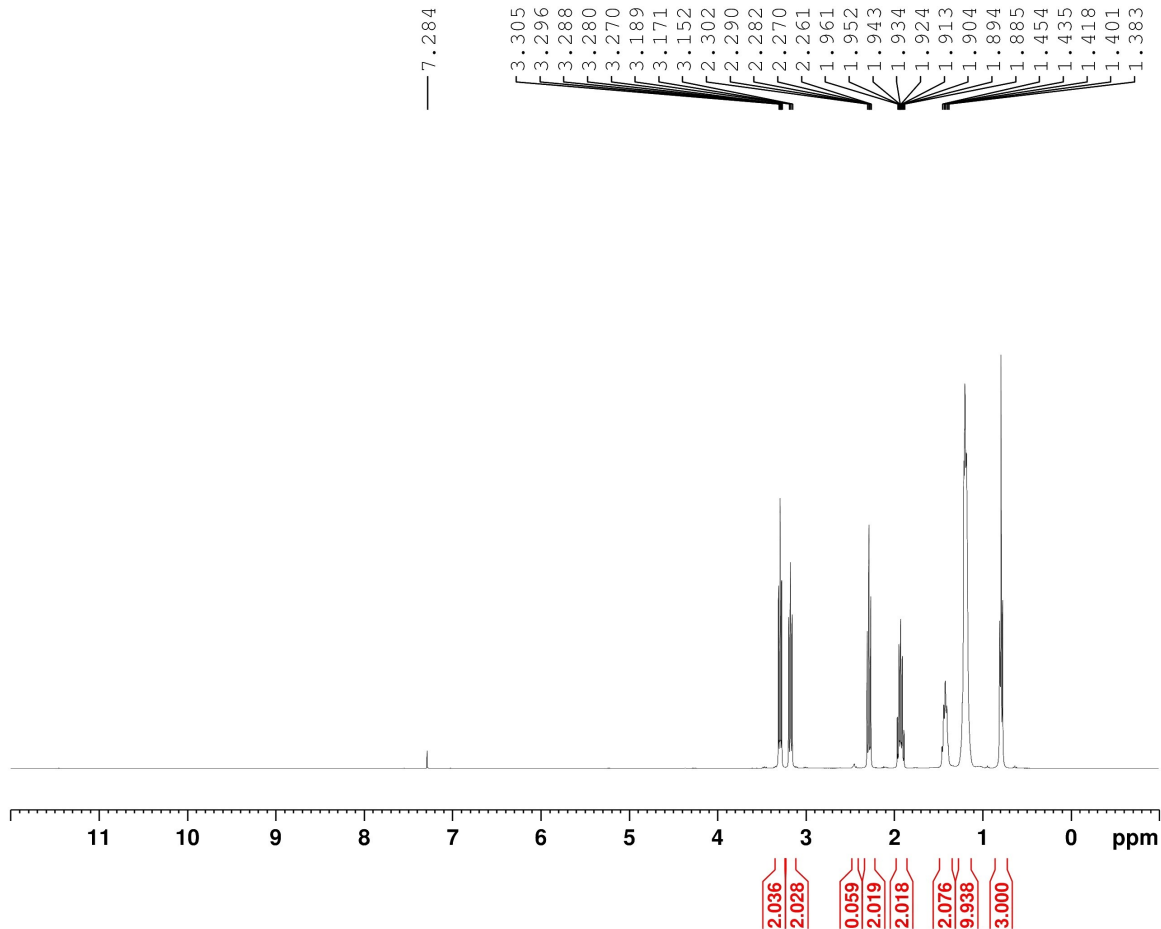

Current Data Parameters
 NAME 2687-94-7P2525078
 EXFNO 1
 PROCNO 1

F2 - Acquisition Parameters
 Date_ 20230217
 Time 17.17 h
 INSTRUM Avance neo 400
 PROBHD Z163739_0670 (
 PULPROG zg30
 TD 65536
 SOLVENT CDCl3
 NS 4
 DS 2
 SWH 8196.722 Hz
 FIDRES 0.250144 Hz
 AQ 3.9976959 sec
 RG 12.7
 DW 61.000 usec
 DE 13.89 usec
 TE 299.0 K
 D1 1.00000000 sec
 TD0 1
 SFO1 400.1324708 MHz
 NUC1 1H
 PO 2.67 usec
 P1 8.00 usec
 PLW1 22.77899933 W

F2 - Processing parameters
 SI 65536
 SF 400.1300000 MHz
 WDW EM
 SSB 0
 LB 0.30 Hz
 GB 0
 PC 1.00