

3597-91-9P2543953

7.642
7.622
7.500
7.496
7.482
7.462
7.408
7.405
7.395
7.390
7.385
7.372
7.285

— 4.767


— 1.897



Current Data Parameters
NAME 3597-91-9P2543953
EXFNO 3
PROCNO 1

F2 - Acquisition Parameters
Date_ 20230522
Time 15.18 h
INSTRUM Avance neo 400
PROBHD Z163739_0670 (
PULPROG zg30
TD 65536
SOLVENT CDCl3
NS 4
DS 2
SWH 8196.722 Hz
FIDRES 0.250144 Hz
AQ 3.9976959 sec
RG 90.5
DW 61.000 usec
DE 13.89 usec
TE 297.7 K
D1 1.00000000 sec
TD0 1
SF01 400.1324708 MHz
NUC1 1H
PO 2.67 usec
P1 8.00 usec
PLW1 22.77899933 W

F2 - Processing parameters
SI 65536
SF 400.1300000 MHz
WDW EM
SSB 0
LB 0.30 Hz
GB 0
PC 1.00

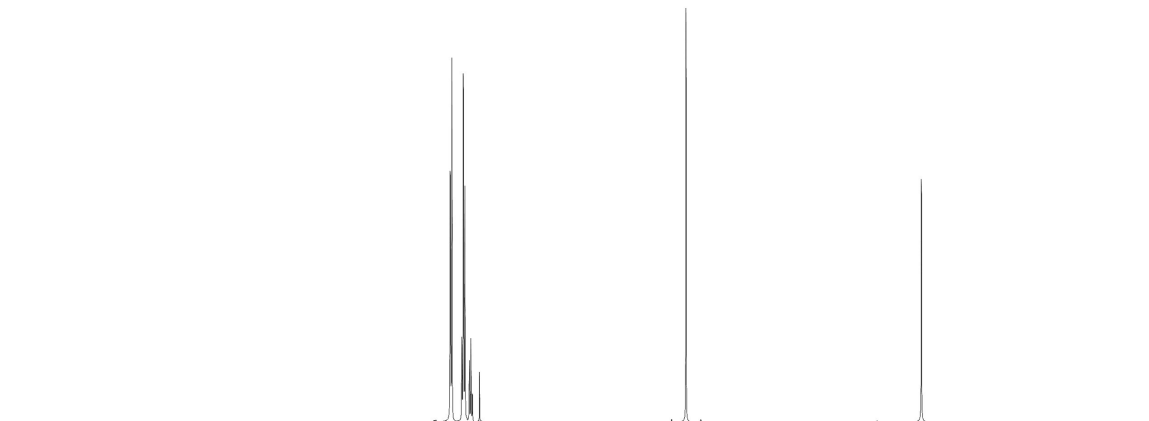

12 11 10 9 8 7 6 5 4 3 2 1 0 ppm

3.945
3.915
0.970

2.000