

38183-12-9P2598627

8.767
8.029
8.010
7.797
7.794
7.778
7.775
7.760
7.757
7.752
7.749
7.731
7.728
7.710
7.527
7.490
7.473
7.455
7.436
7.410
7.397
7.391
7.385
7.373
7.285


— 2.069
— 1.603
— 1.283



Current Data Parameters
NAME 38183-12-9P2598627
EXFNO 1
PROCNO 1

F2 - Acquisition Parameters
Date_ 20230417
Time 10.05 h
INSTRUM Avance neo 400
PROBHD Z163739_0670 (
PULPROG zg30
TD 65536
SOLVENT CDCl3
NS 4
DS 2
SWH 8196.722 Hz
FIDRES 0.250144 Hz
AQ 3.9976359 sec
RG 101
DW 61.000 usec
DE 13.89 usec
TE 297.3 K
D1 1.00000000 sec
TD0 1
SF01 400.1324708 MHz
NUC1 1H
PO 2.67 usec
P1 8.00 usec
PLW1 22.77899933 W

F2 - Processing parameters
SI 65536
SF 400.1300000 MHz
WDW EM
SSB 0
LB 0.30 Hz
GB 0
PC 1.00

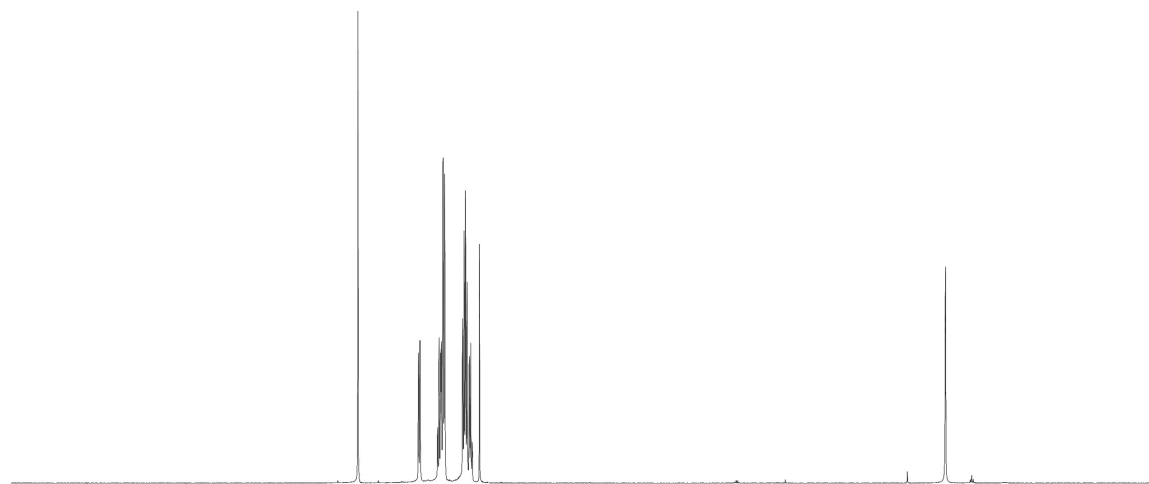

12 11 10 9 8 7 6 5 4 3 2 1 0 ppm

0.966

1.000

4.102

4.055

0.023

0.047