

41459-42-1P2024745


— 9.666

— 7.263

— -0.000



3.824
3.811
3.797
3.785
3.763
3.747
3.736
3.720
3.287
3.275
3.272
3.259
3.247
3.243
3.231

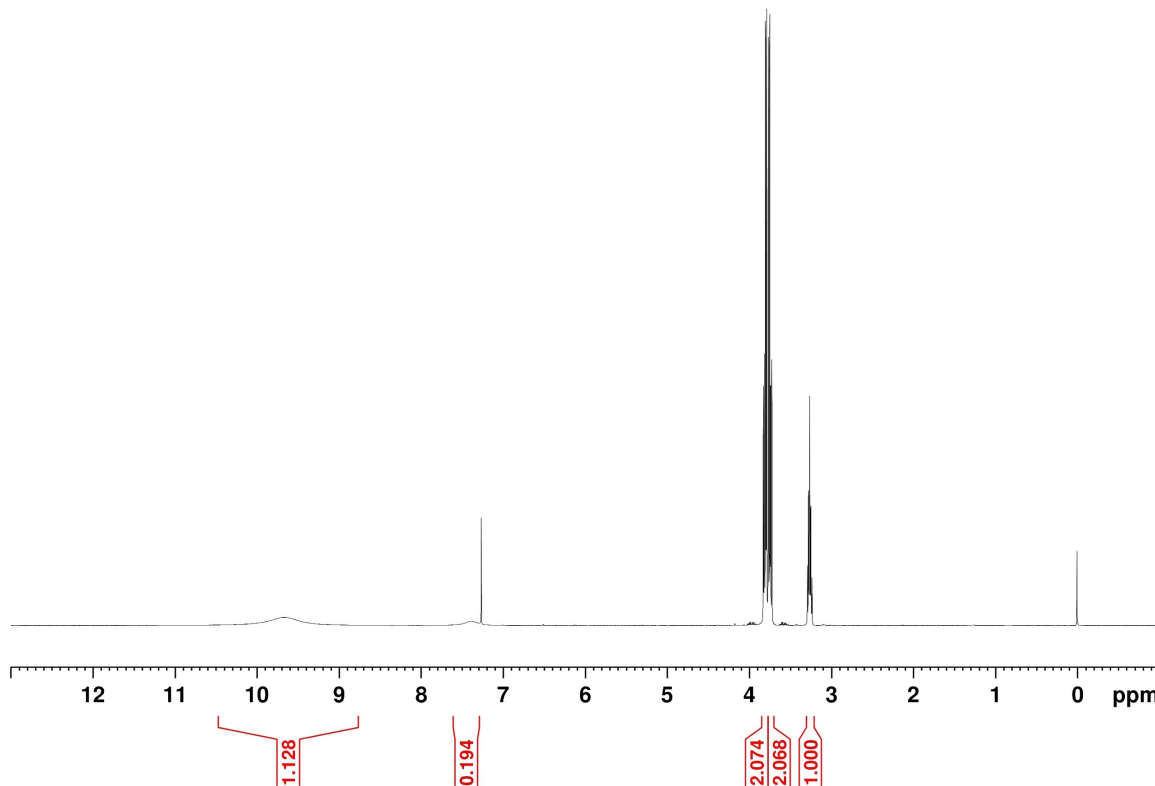

Current Data Parameters
NAME 41459-42-1P2024745
EXPNO 1
PROCNO 1

F2 - Acquisition Parameters
Date_ 20231031
Time 17.03 h
INSTRUM Avance neo 400
PROBHD Z163739_0670 (
PULPROG zg30
TD 65536
SOLVENT CDCl3
NS 4
DS 2
SWH 8196.722 Hz
FIDRES 0.250144 Hz
AQ 3.9976359 sec
RG 101
DW 61.000 usec
DE 13.89 usec
TE 297.3 K
D1 1.00000000 sec
TD0 1
SF01 400.1324708 MHz
NUC1 1H
PO 2.67 usec
P1 8.00 usec
PLW1 22.77899933 W

F2 - Processing parameters
SI 65536
SF 400.1300086 MHz
WDW EM
SSB 0
LB 0.30 Hz
GB 0
PC 1.00