

4478-93-7P2862719


3.640
3.625
3.610
2.770
2.760
2.754
2.742
2.735
2.724
2.709
2.609
2.023
1.986
1.980
1.968
1.962
1.944
1.937
1.933
1.929
1.924
1.921
1.908
1.888



Current Data Parameters
NAME 4478-93-7P2862719
EXFNO 1
PROCNO 1

F2 - Acquisition Parameters
Date_ 20231207
Time 11.23 h
INSTRUM Avance neo 400
PROBHD Z163739_0670 (
PULPROG zg30
TD 65536
SOLVENT CDCl3
NS 4
DS 2
SWH 8196.722 Hz
FIDRES 0.250144 Hz
AQ 3.9976959 sec
RG 32
DW 61.000 usec
DE 13.89 usec
TE 297.5 K
D1 1.00000000 sec
TD0 1
SFO1 400.1324708 MHz
NUC1 1H
PO 2.67 usec
P1 8.00 usec
PLW1 22.77899933 W

F2 - Processing parameters
SI 65536
SF 400.1299771 MHz
WDW EM
SSB 0
LB 0.30 Hz
GB 0
PC 1.00

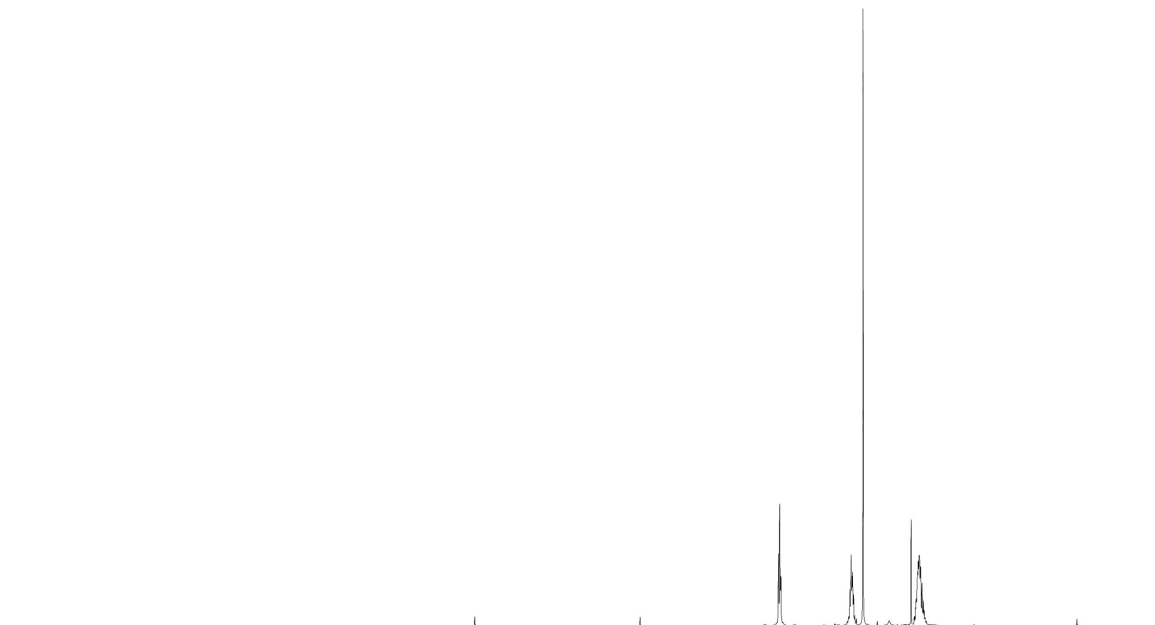

12 11 10 9 8 7 6 5 4 3 2 1 0 ppm

0.055

2.025

2.058

3.000

0.447

4.002