

504-15-4P2701779


— 7.285
6.264
6.260
6.194
6.189
6.184
— 4.792
— 2.268
— 1.678



Current Data Parameters
NAME 504-15-4P2701779
EXFNO 1
PROCNO 1

F2 - Acquisition Parameters
Date_ 20230721
Time 13.23 h
INSTRUM Avance neo 400
PROBHD Z163739_0670 (
PULPROG zg30
TD 65536
SOLVENT CDCl3
NS 4
DS 2
SWH 8196.722 Hz
FIDRES 0.250144 Hz
AQ 3.9976359 sec
RG 101
DW 61.000 usec
DE 13.89 usec
TE 296.1 K
D1 1.00000000 sec
TD0 1
SFO1 400.1324708 MHz
NUC1 1H
PO 2.67 usec
P1 8.00 usec
PLW1 22.77899933 W

F2 - Processing parameters
SI 65536
SF 400.1300000 MHz
WDW EM
SSB 0
LB 0.30 Hz
GB 0
PC 1.00

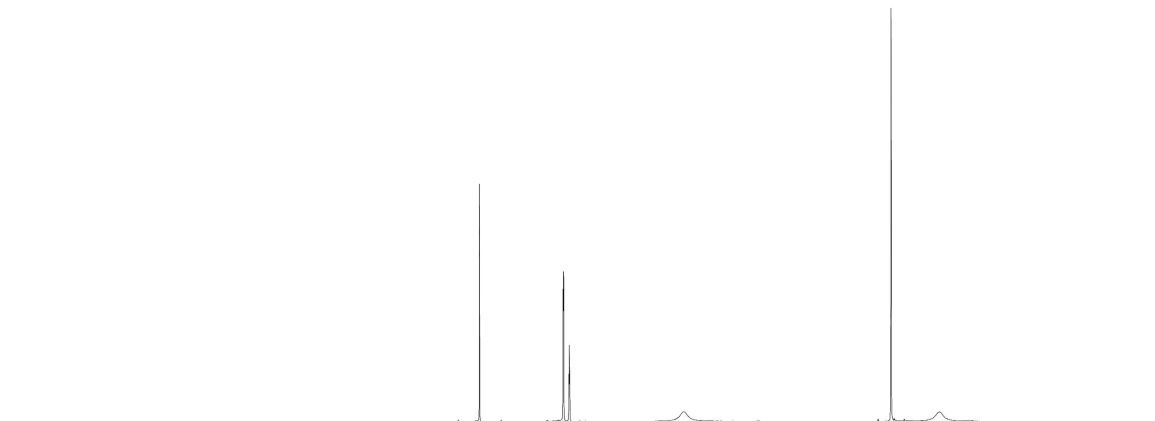

12 11 10 9 8 7 6 5 4 3 2 1 0 ppm

2.060
1.000
1.798
3.207