

5223-06-3P2555889

8.309
7.451
7.447
7.431
7.427
7.285
7.090
7.070


4.505
4.003
3.988
3.974
2.986
2.971
2.957
2.636
2.617
2.598
2.579
1.244
1.225
1.206



Current Data Parameters
NAME 5223-06-3P2555889
EXFNO 4
PROCNO 1

F2 - Acquisition Parameters
Date_ 20230330
Time 10.59 h
INSTRUM Avance neo 400
PROBHD Z163739_0670 (
PULPROG zg30
TD 65536
SOLVENT CDCl3
NS 4
DS 2
SWH 8196.722 Hz
FIDRES 0.250144 Hz
AQ 3.9976959 sec
RG 32
DW 61.000 usec
DE 13.89 usec
TE 297.4 K
D1 1.00000000 sec
TD0 1
SF01 400.1324708 MHz
NUC1 1H
PO 2.67 usec
P1 8.00 usec
PLW1 22.77899933 W

F2 - Processing parameters
SI 65536
SF 400.1300000 MHz
WDW EM
SSB 0
LB 0.30 Hz
GB 0
PC 1.00

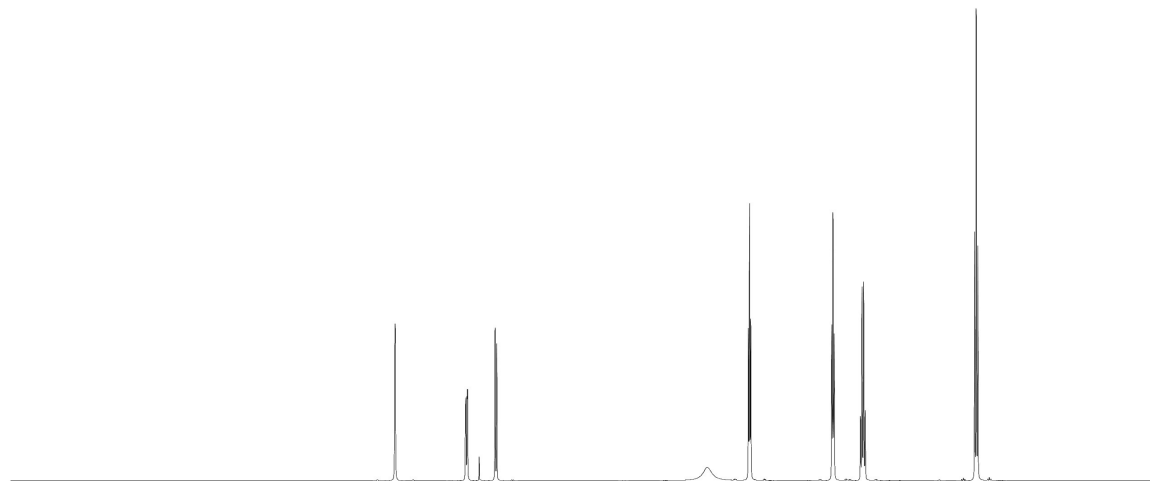

12 11 10 9 8 7 6 5 4 3 2 1 0 ppm

1.000

1.011

1.020

0.965

2.115

2.111

2.084

3.110