

6315-52-2P2559848

7.754
7.733
7.363
7.343
7.284

4.196

2.467


1.689



Current Data Parameters
NAME 6315-52-2P2559848
EXFNO 1
PROCNO 1

F2 - Acquisition Parameters
Date_ 20230322
Time 11.30 h
INSTRUM Avance neo 400
PROBHD Z163739_0670 (
PULPROG zg30
TD 65536
SOLVENT CDCl3
NS 4
DS 2
SWH 8196.722 Hz
FIDRES 0.250144 Hz
AQ 3.9976959 sec
RG 64
DW 61.000 usec
DE 13.89 usec
TE 296.7 K
D1 1.00000000 sec
TD0 1
SF01 400.1324708 MHz
NUC1 1H
PO 2.67 usec
P1 8.00 usec
PLW1 22.77899933 W

F2 - Processing parameters
SI 65536
SF 400.1300000 MHz
WDW EM
SSB 0
LB 0.30 Hz
GB 0
PC 1.00

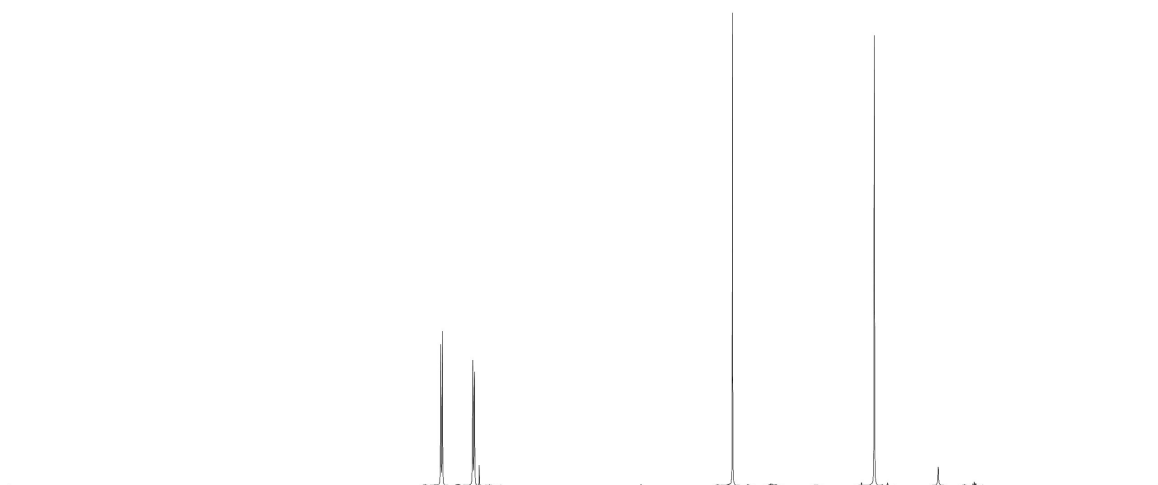

3.819
3.872

4.027
0.053

6.000

0.076