

7158-32-9P1904153

8.214  
8.207  
8.202  
8.190  
8.185  
8.178  
8.164  
8.153  
7.285  
7.194  
7.187  
7.181  
7.176  
7.169  
7.164  
7.157  
7.145  
7.123


2.335  
2.326  
2.284  
1.993  
1.982



Current Data Parameters  
NAME 7158-32-9P1904153  
EXFNO 1  
PROCNO 1

F2 - Acquisition Parameters  
Date\_ 20230828  
Time 15.28 h  
INSTRUM Avance neo 400  
PROBHD Z163739\_0670 (   
PULPROG zg30  
TD 65536  
SOLVENT CDCl3  
NS 4  
DS 2  
SWH 8196.722 Hz  
FIDRES 0.250144 Hz  
AQ 3.9976359 sec  
RG 101  
DW 61.000 usec  
DE 13.89 usec  
TE 299.1 K  
D1 1.00000000 sec  
TD0 1  
SFO1 400.1324708 MHz  
NUC1 1H  
PO 2.67 usec  
P1 8.00 usec  
PLW1 22.77899933 W

F2 - Processing parameters  
SI 65536  
SF 400.1300000 MHz  
WDW EM  
SSB 0  
LB 0.30 Hz  
GB 0  
PC 1.00

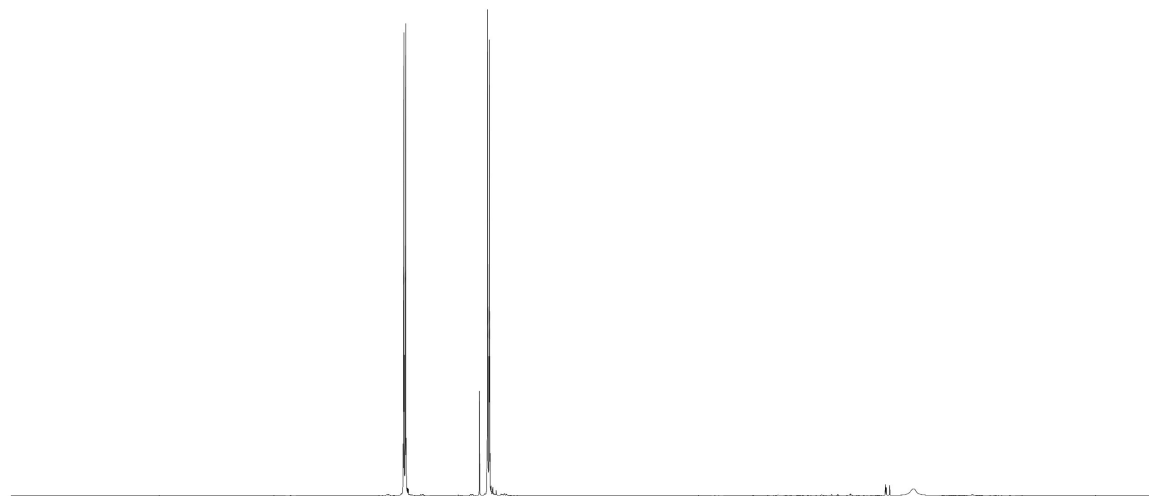

12 11 10 9 8 7 6 5 4 3 2 1 0 ppm

4.000

4.062

0.079

0.037