


7365-45-9P2383496



4.699
3.834
3.821
3.808
3.638
3.624
3.170
3.105
3.098
3.078
3.066
3.020
2.935
2.916

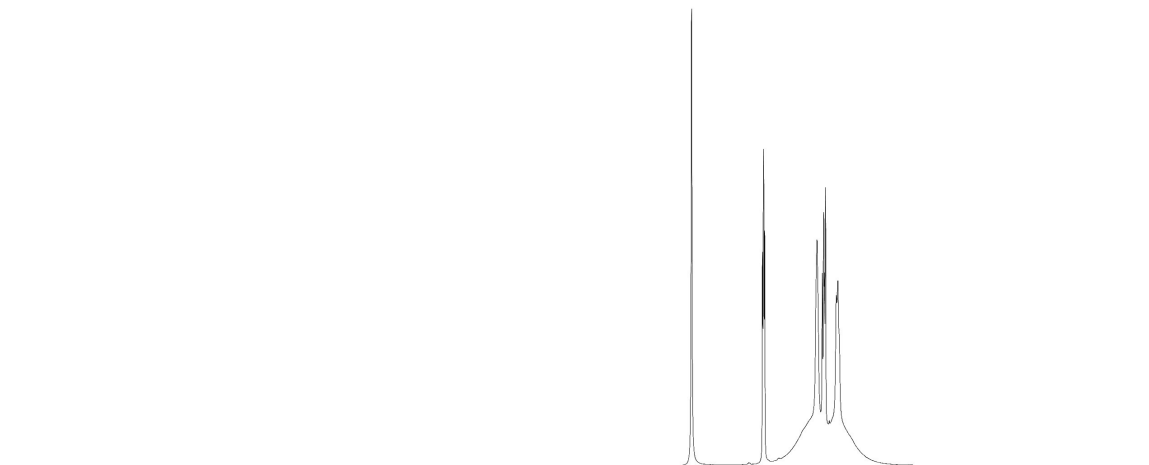

2.070
2.203
3.074
2.911
5.742

Current Data Parameters
NAME 7365-45-9P2383496
EXFNO 1
PROCNO 1

F2 - Acquisition Parameters
Date_ 20240319
Time 11.06 h
INSTRUM Avance neo 400
PROBHD Z163739_0670 (
PULPROG zg30
TD 65536
SOLVENT D2O
NS 4
DS 2
SWH 8196.722 Hz
FIDRES 0.250144 Hz
AQ 3.9976359 sec
RG 45.2
DW 61.000 usec
DE 13.89 usec
TE 297.8 K
D1 1.00000000 sec
TD0 1
SFO1 400.1324708 MHz
NUC1 1H
PO 2.67 usec
P1 8.00 usec
PLW1 22.77899933 W

F2 - Processing parameters
SI 65536
SF 400.1300000 MHz
WDW EM
SSB 0
LB 0.30 Hz
GB 0
PC 1.00