


94-97-3P2498387

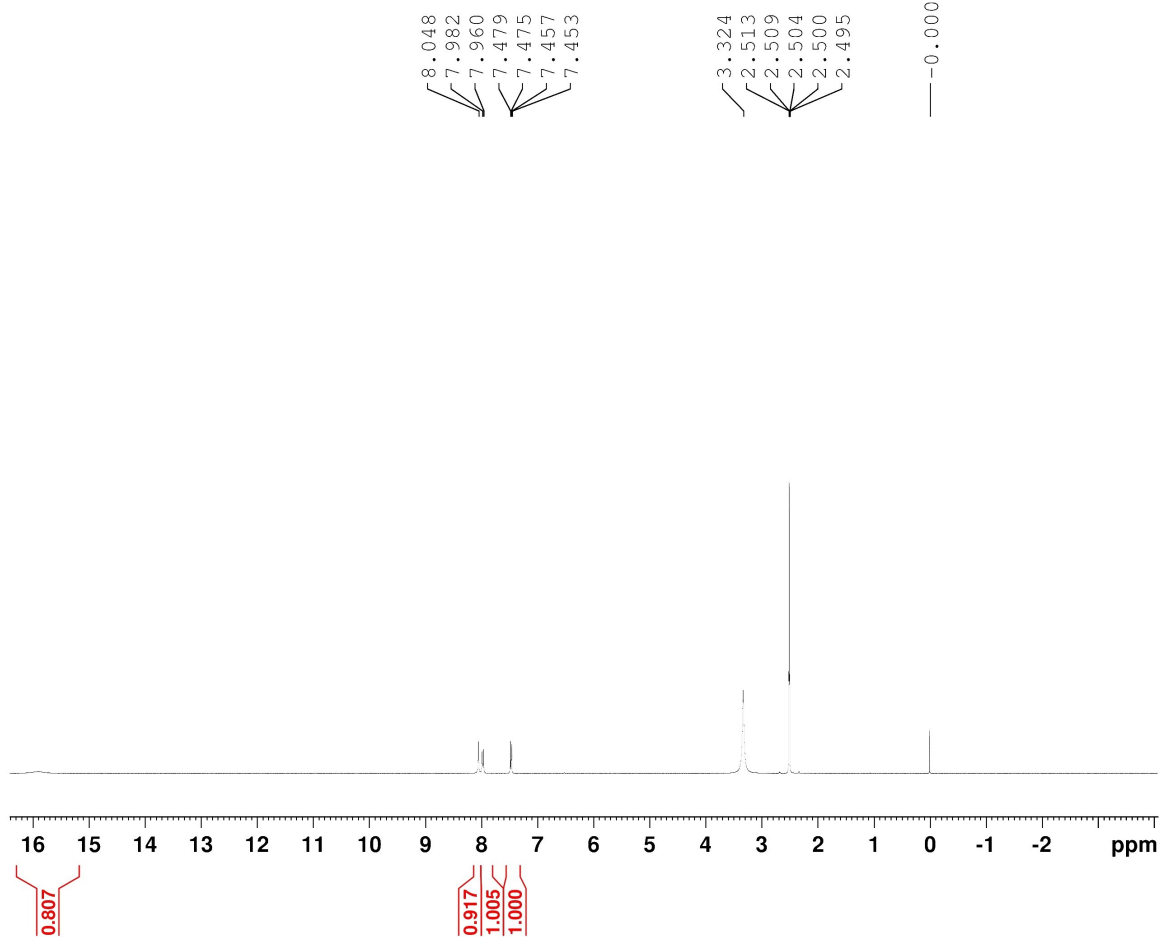

8.048
7.982
7.960
7.479
7.475
7.457
7.453

3.324
2.513
2.509
2.504
2.500
2.495

— 0.000



Current Data Parameters
NAME 94-97-3P2498387
EXFNO 1
PROCNO 1

F2 - Acquisition Parameters
Date_ 20230113
Time 10.07 h
INSTRUM Avance neo 400
PROBHD 2163739_0670 (
PULPROG zg30
TD 65536
SOLVENT DMSO
NS 4
DS 2
SWH 8196.722 Hz
FIDRES 0.250144 Hz
AQ 3.9976359 sec
RG 101
DW 61.000 usec
DE 13.89 usec
TE 299.8 K
D1 1.00000000 sec
TD0 1
SFO1 400.1324708 MHz
NUC1 1H
PO 2.67 usec
P1 8.00 usec
PLW1 22.77899933 W

F2 - Processing parameters
SI 65536
SF 400.1300019 MHz
WDW EM
SSB 0
LB 0.30 Hz
GB 0
PC 1.00